



Precision and reproducibility of T2 quantifications in myocardial T2 mapping: impact of the number of echoes and reconstruction model

Citation

Basha, Tamer, Mehmet Akcakaya, Sébastien Roujol, and Reza Nezafat. 2015. "Precision and reproducibility of T2 quantifications in myocardial T2 mapping: impact of the number of echoes and reconstruction model." *Journal of Cardiovascular Magnetic Resonance* 17 (1): W9. doi:10.1186/1532-429X-17-S1-W9. <http://dx.doi.org/10.1186/1532-429X-17-S1-W9>.

Published Version

doi:10.1186/1532-429X-17-S1-W9

Permanent link

<http://nrs.harvard.edu/urn-3:HUL.InstRepos:14065433>

Terms of Use

This article was downloaded from Harvard University's DASH repository, and is made available under the terms and conditions applicable to Other Posted Material, as set forth at <http://nrs.harvard.edu/urn-3:HUL.InstRepos:dash.current.terms-of-use#LAA>

Share Your Story

The Harvard community has made this article openly available.
Please share how this access benefits you. [Submit a story](#).

[Accessibility](#)

WORKSHOP PRESENTATION

Open Access

Precision and reproducibility of T_2 quantifications in myocardial T_2 mapping: impact of the number of echoes and reconstruction model

Tamer Basha^{1,2*}, Mehmet Akcakaya^{1,2}, Sébastien Roujol^{1,2}, Reza Nezafat^{1,2}

From 18th Annual SCMR Scientific Sessions
Nice, France. 4-7 February 2015

Background

Quantitative myocardial T_2 is a promising technique to assess myocardial inflammation and edema (1). Recent implementations have utilized T_2 -prepared (T_2 prep) SSFP sequences to acquire a multiple T_2 weighted images at different echo times, and generate T_2 maps based on a 2-parameter (2P-fit) model of T_2 decay (2,3). Recently, a 3-parameter fitting (3P-fit) model was found superior to the conventional 2P-fit model, as it compensates for T_1 relaxation effect, and results in more accurate T_2 measurements (4). In this work, we sought to characterize the 3P-fit approach in terms of precision and reproducibility and to evaluate the influence of the number of employed T_2 prep echo times on these two metrics.

Methods

Monte-Carlo simulations (1000 repetitions) were performed to study the effect of increasing the number of T_2 prep images. Block equation was used to simulate the signal intensities of a presumed tissue of $T_2 = 50$ ms at different T_2 prep echo times and different SNR levels. T_2 was then estimated using a 2- and 3-parameter fitting model, and the precision was quantified for each model. Ten healthy subjects (27 ± 10 y/o, 5m) were then imaged using a 1.5 T Phillips scanner with a free-breathing ECG-triggered single shot T_2 prep bSSFP sequence (FOV = 320×320 mm², in-plane resolution = 2.5×2.5 mm², slice thickness = 8mm, TR/TE = 2.2/1.1ms, FA = 40°, SENSE rate = 2, acquisition window = 140 ms, 14 T_2 prep echo times = 0,25,35,...135,145 ms). A 4s rest period after each image to allow for full spin relaxation.

Data were reconstructed using the 3P-fit model. For comparison, a conventional T_2 mapping sequence was acquired (Breath hold, 3 T_2 prep echo times = 20,50,75ms, and 2P-fit model). For each subject, both sequences were repeated 5 times. Precision and reproducibility were compared using different subset of T_2 prep echo times. Based on these results, an optimized T_2 mapping sequence using 10 T_2 prep echoes and a 3P-fit model is proposed and evaluated in-vivo in 10 healthy subjects (29 ± 17 y/o, 4m). This sequence is compared to the same conventional T_2 mapping sequence in term of precision and reproducibility.

Results

T_2 measurements using a 2P-fit model are dependent on the number of T_2 prep echo times (Figure 1). The 3P-fit model provides T_2 measurements independent from the number of T_2 prep echo times. Higher precision and reproducibility was achieved with increased number of T_2 prep echo times. Improved in-vivo precision and reproducibility was achieved using the proposed sequence when compared to the conventional sequence (7ms vs. 11ms $p=XX$ and 1.2ms vs. 2.4ms $p=XX$, respectively) (Figure 2).

Conclusions

The proposed sequence using 10 T_2 prep echo times and a 3P-fit model is independent from the number of T_2 prep echo times and provides better in-vivo precision and reproducibility than the conventional technique.

Funding

N/A.

¹Cardiology, BIDMC, Boston, MA, USA

Full list of author information is available at the end of the article

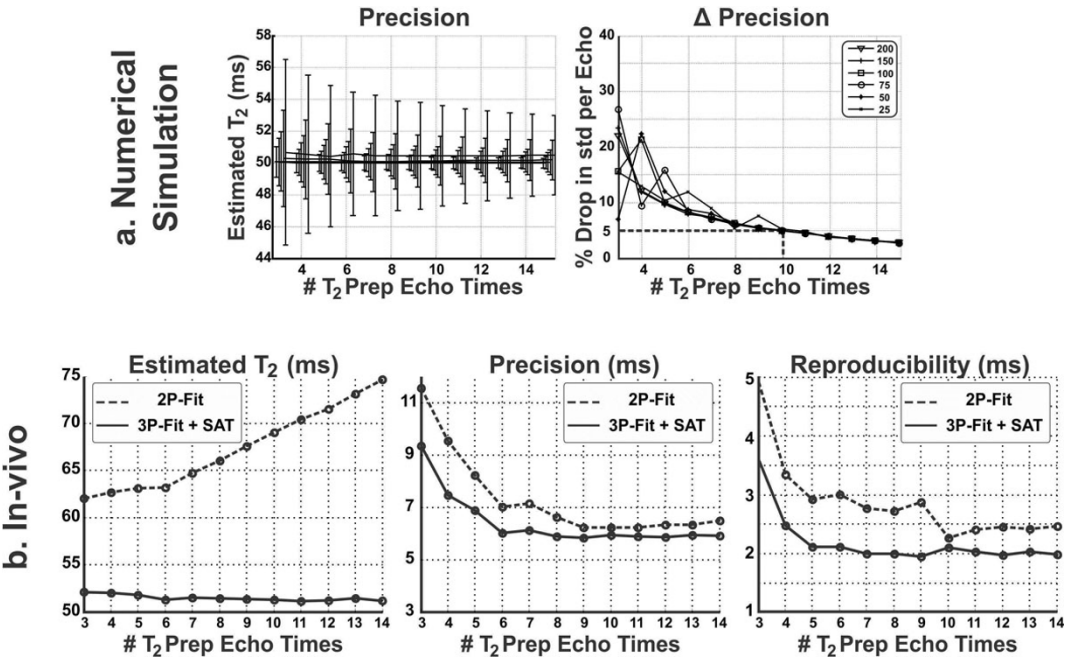


Figure 1 a) Numerical simulation results for the effect of number of echo images on the precision of the quantifications for different signal-to-noise ratios. As the number of echoes increases, the precision gets better till it nearly saturates for number of echoes ≥ 10 . b) Accuracy, precision and reproducibility of T_2 mapping when using different number of echo images. With increasing the number of echoes, estimated T_2 values changes significantly when using 2-pt fits, while it shows consistency when using the 3-pt fits regardless of the number of echoes used for the estimation. Both precision and reproducibility increases when using more echo images for the T_2 estimation. However, and similar to what numerical simulations predicts, the effect nearly saturates for number of echoes ≥ 10 .

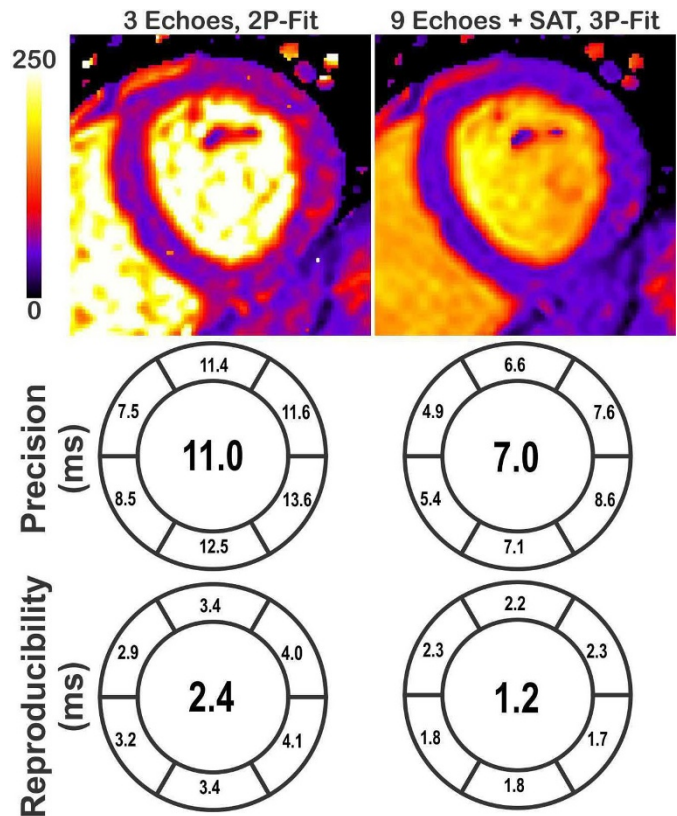


Figure 2 An example for the T_2 maps of one healthy subject. The bull's-eyes shows the overall precision and reproducibility among the 10 subject in a segment-based analysis, when using the 3 echoes with 2-pt fit, and 10 echoes with 3-pt fit.

Authors' details

¹Cardiology, BIDMC, Boston, MA, USA. ²Harvard Medical School, Boston, MA, USA.

Published: 3 February 2015

References

1. He: *JMRI* 2006.
2. Giri: *MRM* 2012.
3. Van Heeswijk: *JACC* 2012.
4. Akçakaya: *MRM* 2014.

doi:10.1186/1532-429X-17-S1-W9

Cite this article as: Basha et al.: Precision and reproducibility of T₂ quantifications in myocardial T₂ mapping: impact of the number of echoes and reconstruction model. *Journal of Cardiovascular Magnetic Resonance* 2015 **17**(Suppl 1):W9.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

